


# Soft Sensors, 8000S Series



## Two Sensors in One


The Nonin soft sensor offers ultimate flexibility for SpO<sub>2</sub> monitoring – whether short term spot checking or continuous monitoring. The specially designed soft sensors offer superior patient comfort by providing an optimal distribution of pressure and three models to fit a variety of patient hands – children to adult. The Nonin soft sensors with trusted PureLight® technology, combined with Nonin's PureSAT® signal processing, provide consistent results – patient to patient and sensor to sensor, even under challenging patient conditions such as motion and low perfusion.

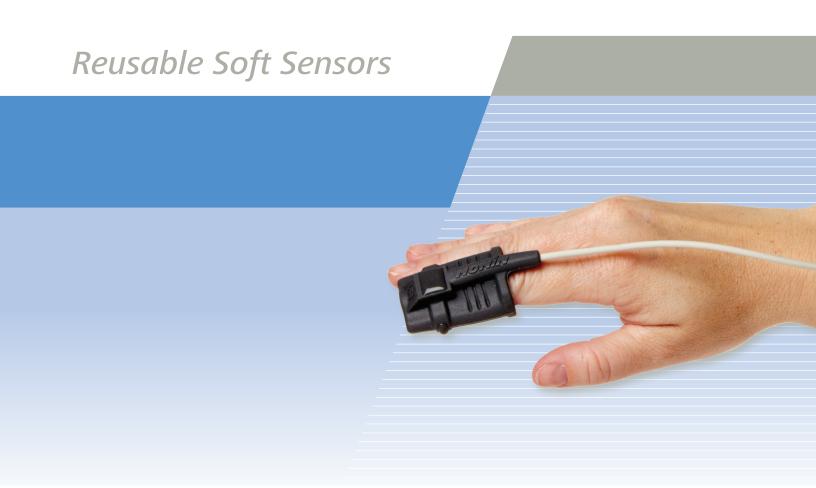

# 8000S Series

## **Product Highlights**

- Designed for ultimate comfort short or longer term monitoring
- Suitable for settings where SpO<sub>2</sub> monitoring is required
- Meets all required regulatory and quality standards, including ISO 9919
- Durable silicone material
- Latex free
- Added flexibility for a secure fit

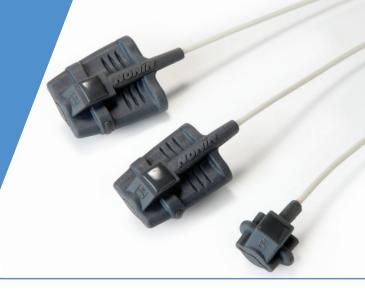

#### **Select Your Size**

#### 8000SL Large<sup>†</sup>



Digit thickness: 12.5mm to 25.5mm (0.5in to 1in) Preferred application: Fingers, Toes

## 8000SM Medium<sup>†</sup>



Digit thickness: 10mm to 19mm (0.4in to 0.75in) Preferred application: Fingers, Toes

#### 8000SS Small<sup>†</sup>



Digit thickness: 7.5mm to 12.5mm (0.3in to 0.5in) Preferred application: Fingers, Toes

†All sizes available in1m/3m/WristOx<sub>2</sub>. Use only with Nonin pulse oximeters.

## WristOx<sub>2</sub>, Model 3150 version

The WristOx<sub>2</sub><sup>™</sup>, Model 3150 features a new ergonomic design and Bluetooth® wireless technology eliminate the inconvenience of bulky cables and provide patients with increased comfort and independence making this pulse oximeter ideal for ambulatory monitoring.



### Specifications\*

SpO<sub>2</sub> Low Perfusion Accuracy (A<sub>rms</sub>\*\*)......70 – 100% ±2 digits<sup>1</sup> Motion\* ..... ±3 digits Pulse Rate Low Perfusion Accuracy (A<sub>rms</sub>\*\*) ........ 40 – 240 BPM ±3 digits<sup>1</sup> **Temperature** 

Storage/Transportation .....-30 °C to +70 °C (-22 °F to +158 °F)

#### Humidity

This product complies with ISO 10993-1

<sup>1</sup>Additional accuracy and performance information can be found in the pulse oximeter operator's manual. <sup>2</sup>Accuracy testing was performed under no-motion conditions.

\*See product Instructions for Use (IFU) for more information on product specifications and testing. \*\* ±1 A<sub>rms</sub> encompasses 68% of the population. This information is especially useful for clinicians performing

Specifications are subject to change without notice.

#### Nonin Medical, Inc.

13700 1st Avenue North Plymouth, MN = 55441-5443 = USA P +1.763.553.9968 TF 800.356.8874

F+1.763.577.5521 E info@nonin.com

#### www.nonin.com



Nonin Medical AB Fibervägen 2, 82450

Hudiksvall, Sweden

P +46 650 401500 F +46 650 401514

E infointl@nonin.se





